

OSSERVATORIO ASTROFISICO DI CATANIA

Characterization Test of SiPM SensL

Device: J-Series

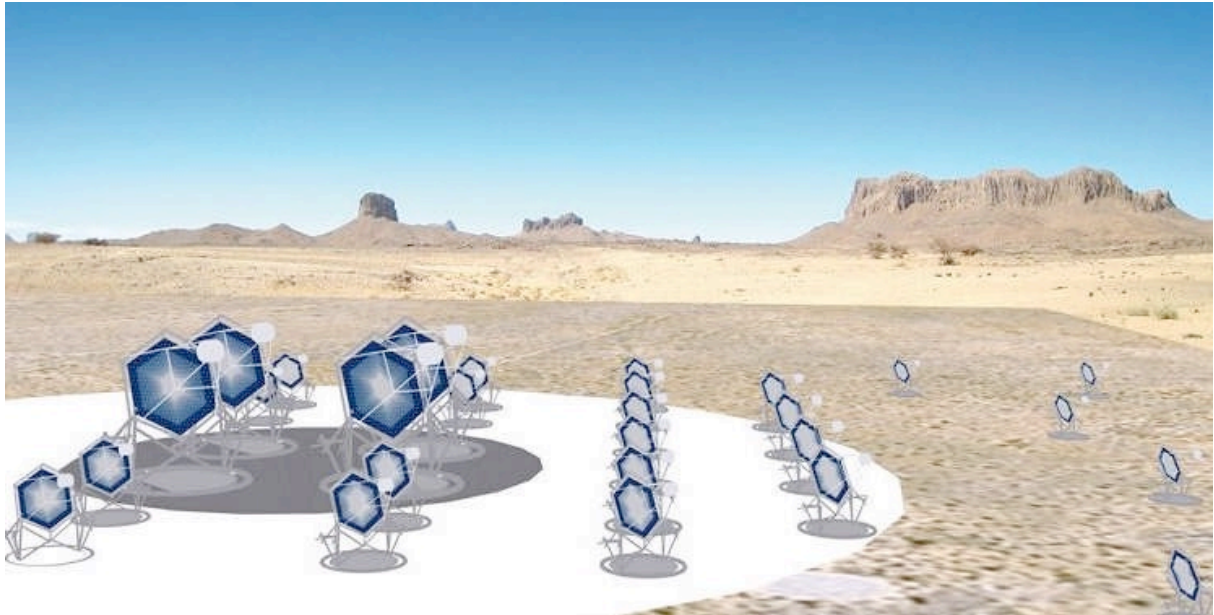

Osservatorio Astrofisico di Catania

G. ROMEO⁽¹⁾

(1) INAF - Osservatorio Astrofisico di Catania

Rapporti interni e tecnici
N.11/2015

INAF - Osservatorio Astrofisico di Catania


Via Santa Sofia, 78 I-95123 Catania, Italy Tel.: +39-095-7332 111 Fax: +39-095-330592


Sede "Mario G.Fracastoro" (Etna) - Tel +39-095-911580 Fax+39-095-916184

www.oact.inaf.it - oacatania@oact.inaf.it

Characterization Test of SiPM SensL J-Series

Measures of: Dark Stairs, Dark Count Rate and Cross-Talk

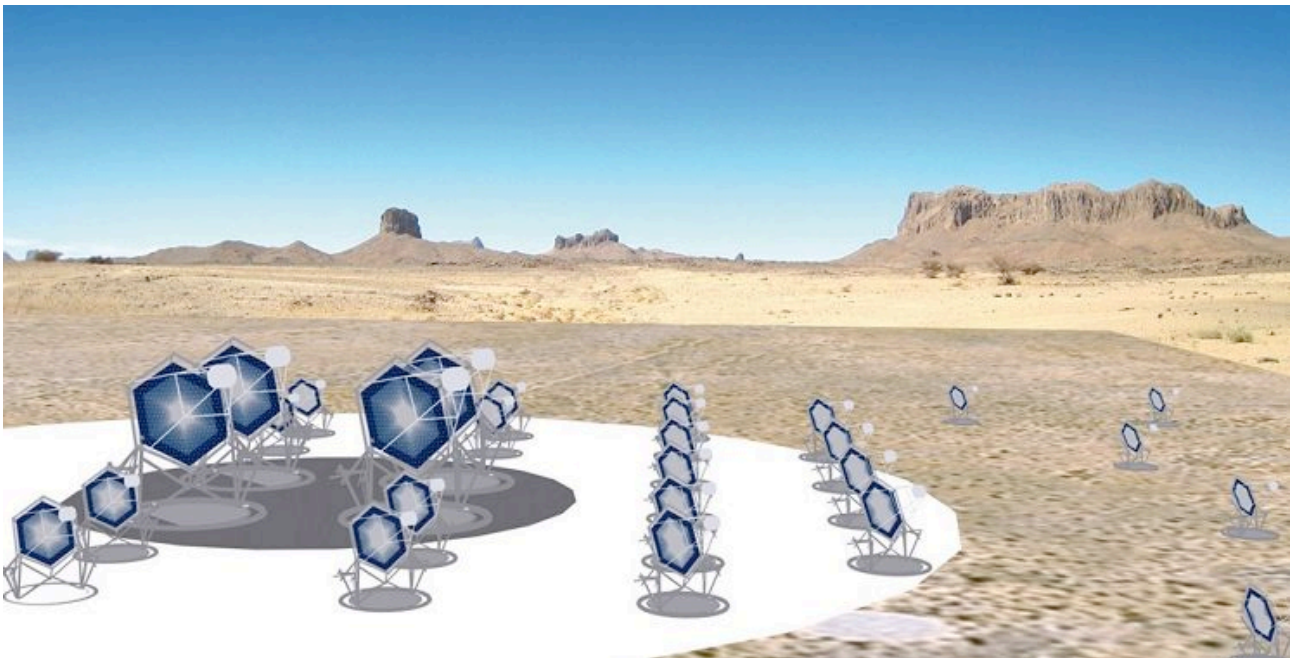

Prepared by: Name: Giuseppe Romeo Signature:  Date: 30/07/2015

Reviewed by: Name: Giovanni Bonanno Signature  Date: 30/07/2015

Approved by: Name: Giovanni Bonanno Signature:  Date: 30/07/2015

TABLE OF CONTENTS

DISTRIBUTION LIST	3
LIST OF ACRONYMS	4
1. INTRODUCTION	5
2. MEASUREMENT SYSTEM	6
3. Electrical Characteristics and Physical from Data Sheet.....	8
4. Measurements Results	9
5. CONTACTS	12



DISTRIBUTION LIST

ASTRI mailing list	astri@brera.inaf.it
Bruno Sacco	bruno.sacco@iasf-palermo.inaf.it
Giovanni Pareschi	giovanni.pareschi@brera.inaf.it
Stefano Vercellone	stefano@ifc.inaf.it
Rodolfo Canestrari	rodolfo.canestrari@brera.inaf.it
Osvaldo Catalano	osvaldo.catalano@iasf-palermo.inaf.it
Enrico Cascone	cascone@na.astro.it
Giovanni La Rosa	larosa@ifc.inaf.it
Giovanni Bonanno	gbo@oact.inaf.it
Giuseppe Romeo	giuseppe.romeo@oact.inaf.it
Domenico Impiombato	domenico.impiombato@ifc.inaf.it
Patrizia Caraveo	pat@lambrate.inaf.it
Davide Marano	davide.marano@oact.inaf.it
Alessandro Grillo	agrillo@oact.inaf.it
Luca Stringhetti	luca@iasf-milano.inaf.it
Rachele Millul	rachele.millul@brera.inaf.it
Mauro Fiorini	fiorini@lambrate.inaf.it
Salvatore Garozzo	salvatore.garozzo@oact.inaf.it
Giuseppe Sottile	sottile@ifc.inaf.it
Salvatore Giarrusso	jerry@ifc.inaf.it
ASTRI mailing list	astri@brera.inaf.it



LIST OF ACRONYMS

OACT	Osservatorio Astrofisico di Catania
IFC	Istituto di Astrofisica Spaziale e Fisica Cosmica di Palermo
COLD	Catania astrophysical Observatory Laboratory for Detectors
PCB	Printed Circuit Board
SiPM	Silicon Photo-Multiplier
MPPC	Multi Pixel Photon Counter
SST-2M	Small-Size Telescope Dual-Mirror
PDM	Photon Detection Module
ASIC	Application Specific Integrated Circuit
FEE	Front-End Electronics
BEE	Back-End Electronics
FPGA	Field Programmable Gate Array
EASIROC	Extended Analogue Silicon-pm Integrated Read-Out Chip
CITIROC	Cherenkov Imaging Telescope Integrated Read-Out Chip
I/F	Interface
LCT	Low Cross Talk
PSAU	Power Supply and Amplification Unit



1. INTRODUCTION

This document discusses on some measurement results of the SiPM most relevant characteristics: dark stairs, cross-talk (XTalk) and dark count rate (DCR), carried out at the Catania astrophysical Observatory Laboratory for Detectors (COLD) on a class of recently available detectors by SensL.

2. MEASUREMENT SYSTEM

A Xenon lamp is used as a radiation source; a wavelength selection system constituted by a set of band-pass filters and mirrors, and a Czerny-Turner monochromator are exploited to achieve the desired wavelength in the 130-1100nm spectral range, with a FWHM smaller than 1nm. A beam splitter is employed to direct the monochromatic radiation through an optical lens towards an integrating sphere, which hosts, in one port, a 1-cm² NIST-traced reference photodiode and, in a second port, the SiPM sensor to be characterized. The photon flux intensity coming into the integrating sphere can be regulated by means of neutral density filters or changing the aperture of the entrance or exit slits of the monochromator. Due to the small dimensions of the detectors to be characterized with respect to the optical beam, the integrating sphere is used to spatially integrate the radiant flux. Furthermore, appropriate mechanical structures are realized, in terms of both aperture and distance from the centre of the sphere, to illuminate the SiPM detector and the NIST-traced photodiode with the same radiant flux. The reference photodiode allows to evaluate the number of photons per unit area, and then, after a proper rescaling, the number of photons impinging on the detectors under test.

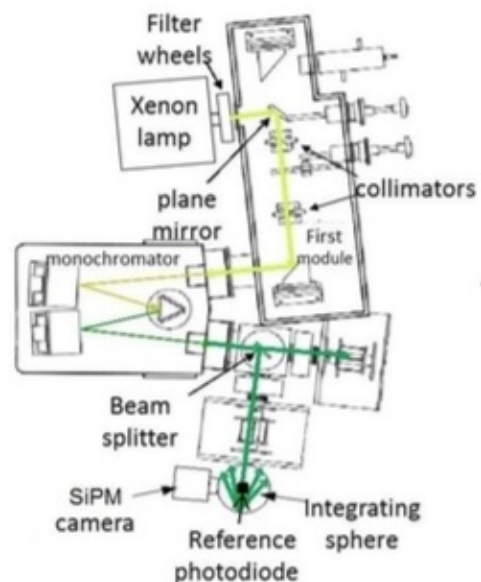
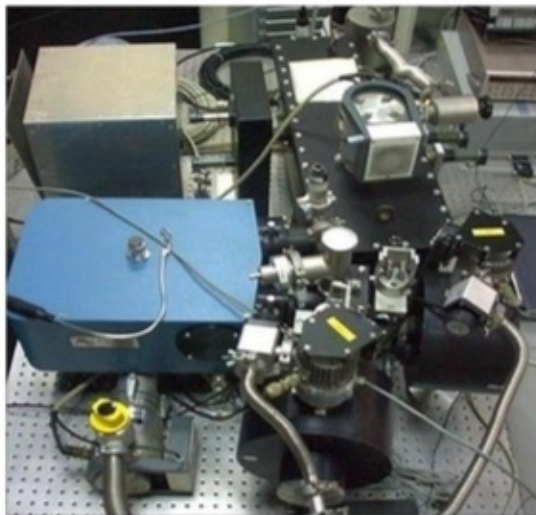


Figure 1. Simplified schematization of the COLD optical apparatus. On the left side: photograph of the characterization equipment. On the right side: scheme of the implemented mechanical and optical parts of the apparatus, where the green line indicates the light path.

The SiPM front-end electronics is a power supply and amplification unit (PSAU), produced by CAEN Electronics, and a two-channel digitizer (Figure 2). The PSAU is an electronic system embedding a power supply and a tunable amplification unit. It provides the cathode voltage for the SiPM detector in a range of 0–120 V with a 16 bit resolution, and features a variable amplification factor up to 50 dB. It integrates a feedback circuit to stabilize the operating voltage (and, in turn, the sensor gain) against thermal variations and a leading edge discriminator feeding an internal counter. In addition, the system can provide a digital output with a tunable width from 20 ns to 320 ns. All parameters can be programmed and monitored via a standard USB interface. An additional holder interface has been implemented for the SiPM electrical board to be connected to the PSAU, and a mechanical cooling adapter has also been realized, allowing to operate the SiPM from room temperatures down to 10°C.

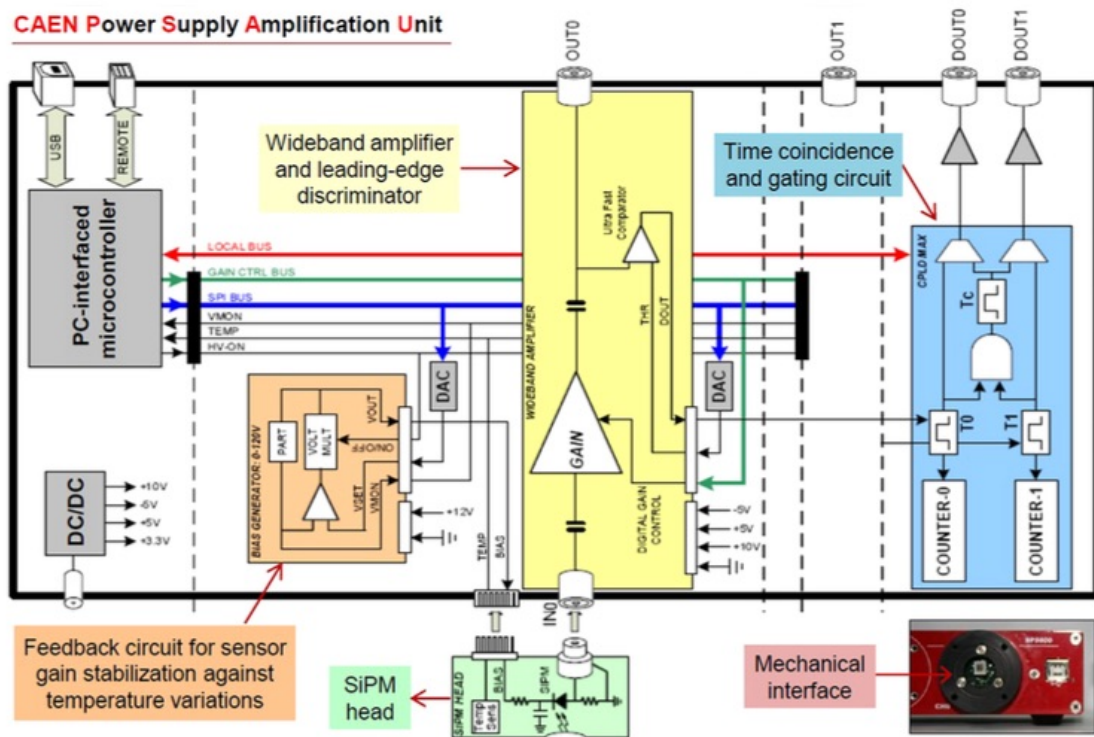


Figure 2. Simplified electric schematization of the power supply and amplification unit.

3. Electrical Characteristics and Physical from Data Sheet.

The characterized SiPM detector presented in this report is the latest device series manufactured by SensL. The following table reports the main physical features of the characterized detector.

<i>Device Series</i>	<i>J-Series</i>
<i>device size</i>	6×6mm ²
<i>fill factor</i>	76%
<i>Breakdown voltage</i>	24.5V
<i>cell pitch</i>	35μm

4. Measurements Results

Staircase and Cross-Talk Measurements

Dark current and optical cross-talk are the main crucial parameters affecting the performance of SiPM detectors. The Dark Count Rate (DCR) is defined as the number of avalanche current pulses produced by thermally generated carriers simulating the detection of single photons at a certain bias voltage. Since the dark noise is comprised of a series of time pulses, its magnitude is often quoted as a pulse rate, typically expressed in kHz or MHz.

It is extremely important that the SiPM operating conditions are maintained stable versus the working temperature during the measurements. The dark signal is amplified and discriminated, generating a logic output pulse each time a dark pulse crosses a predefined voltage level, allowing to select the appropriate threshold.

Optical cross-talk occurs when optical photons that are emitted by accelerated charge carriers undergoing an avalanche propagate towards neighboring diode pixels where, depending on their energy and location, they have a certain probability to generate an additional Geiger avalanche discharge; as a consequence, since the original and neighbor avalanches may occur almost simultaneously (on the same scale of few nanoseconds), single absorbed photons may generate output signals equivalent to more than 1-pe (photoelectron) avalanche events. The experimental approach used for assessing the SiPM cross-talk probability relies on the analysis of DCR measurement results. The SiPM optical cross-talk is evaluated from the DCR data as the ratio between the first and the second event count rate.

In Figure 3, Figure 4 and Figure 5 are shown the staircase, cross-talk and DCR at 15°C and at different overvoltage with the use of the PSAU CAEN.

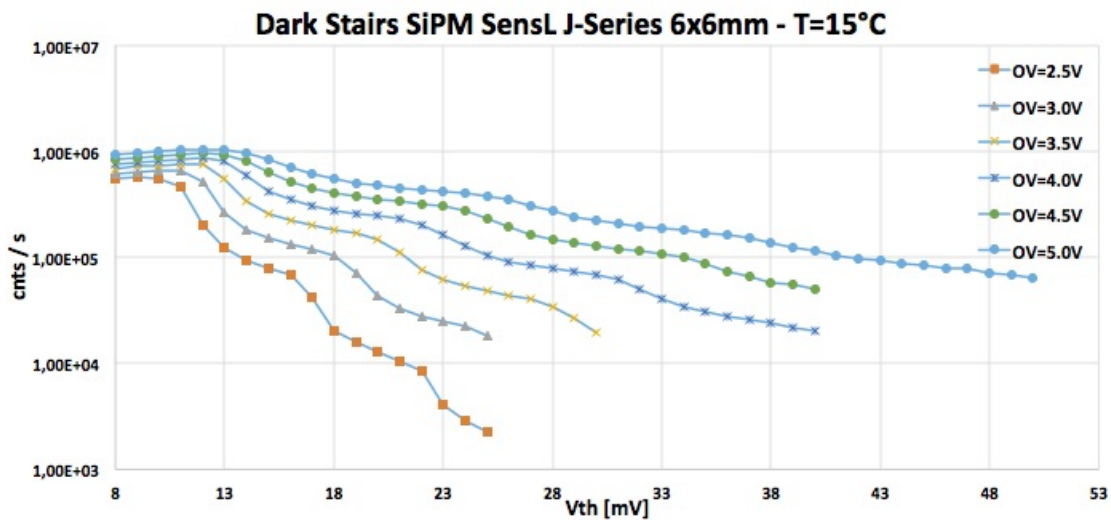


Figure 3. SensL J-Series 6×6mm² Staircase at 15°C and at different overvoltages with the use of the PSAU CAEN.

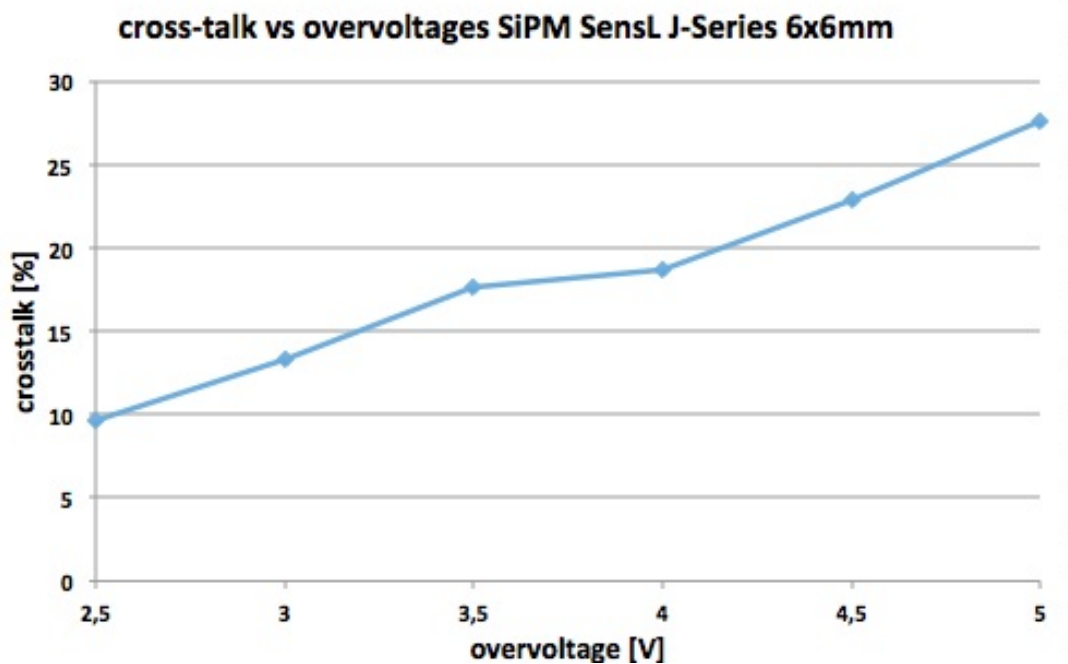


Figure 4. SensL J-Series 6×6mm² Cross-Talk at different overvoltages with the use of the PSAU CAEN.

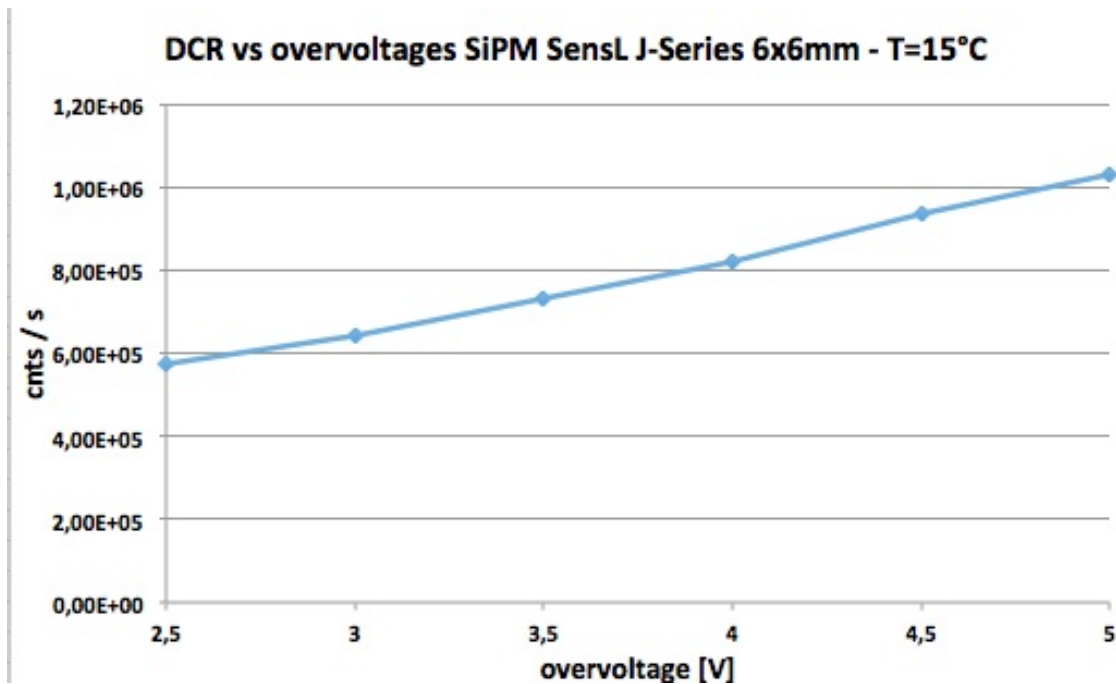


Figure 5. SensL J-Series 6×6mm² Dark Count Rate at different overvoltages with the use of the PSAU CAEN.

All files related to the experimental measurements presented in this report, are located in the database on the PC-LAB (COLD) site Astrophysical Observatory of Catania, path C:\Users\CCDLab1\Desktop\Romeo\Misure

5. CONTACTS

The team working on the electronic design of the ASTRI camera is composed by people from INAF's Catania Astrophysical Observatory and Palermo IFC. It is also referred to as the Electronics Camera Team.

Giovanni Bonanno	gbo@oact.inaf.it	OACT Catania
Giuseppe Romeo	giuseppe.romeo@oact.inaf.it	OACT Catania
Salvatore Garozzo	salvatore.garozzo@oact.inaf.it	OACT Catania
Davide Marano	davide.marano@oact.inaf.it	OACT Catania
Alessandro Grillo	agrillo@oact.inaf.it	OACT Catania
Osvaldo Catalano	osvaldo.catalano@iasf-palermo.inaf.it	IFC Palermo
Giovanni La Rosa	larosa@ifc.inaf.it	IFC Palermo
Giuseppe Sottile	sottile@ifc.inaf.it	IFC Palermo
Salvatore Giarrusso	jerry@ifc.inaf.it	IFC Palermo
Domenico Impiombato	domenico.impiombato@ifc.inaf.it	IFC Palermo