

OSSERVATORIO ASTROFISICO DI CATANIA

SiPM characterization report for the Muon Portal Project

Device: SiPM type P on N - S/N. SPM10H5-60P-Y228159-wf02 ST Microelectronics

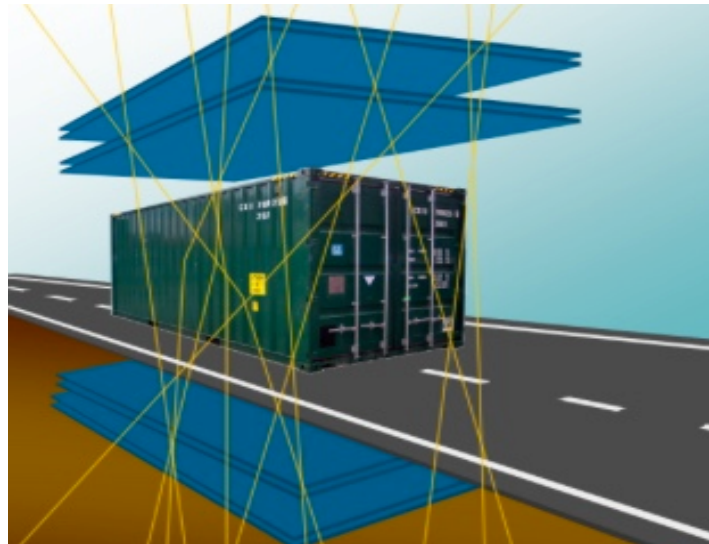

Osservatorio Astrofisico di Catania

G. ROMEO⁽¹⁾, G. BONANNO⁽¹⁾

(1) INAF - Osservatorio Astrofisico di Catania

Rapporti interni e tecnici
N.07/2013

INAF - Osservatorio Astrofisico di Catania

Via Santa Sofia, 78 I-95123 Catania, Italy Tel.: +39-095-7332 111 Fax: +39-095-330592

Sede "Mario G.Fracastoro" (Etna) - Tel +39-095-911580 Fax+39-095-916184

www.oact.inaf.it - oacatania@oact.inaf.it



SiPM CHARACTERIZATION REPORT

OSSERVATORIO ASTROFISICO DI CATANIA
LABORATORIO RIVELATORI



Catania Astrophysical **O**bservatory, **L**aboratory for **D**etectors

Misure eseguite da Giuseppe Romeo

DATE	March 6, 2013
SiPM	ST Microelectronics SiPM type: P on N $V_{BD}=26.71 \text{ V @ } T=25^{\circ}\text{C}$
OP. MODE	Photon Counting with CAEN PSAU and Tektronix counter
SER. N.	SPM10H5-60P - Y228159-wf02



CONTENTS

1.0 Electrical Characteristics from Data sheet.....	3
2.0 Breakdown Voltage	4
4.0 Electro-optical characterization	6
4.1 Characterization at $V_{ov} = 4V$	6
4.1.1 Staircase @ $OV=4V$	6
4.1.2 DCR @ $OV=4V$ at different Gate Time from 25 ns to 110 ns	6
4.1.2 DCR @ $OV=4V$ vs Time.....	7
4.1.4 System linearity to evaluate the best operating conditions	8
4.1.5 PDE measurements at Over-Voltage 4V	9
4.2 Characterization at $V_{ov} = 5V$	10
4.2.1 Staircase @ $OV=5V$	10
4.2.2 DCR @ $OV=5V$ at different Gate Time from 25 ns to 110 ns	10
4.2.3 DCR @ $OV=5V$ vs Time.....	11
4.2.4 System linearity to evaluate the best operating conditions	12
4.2.5 PDE measurements at Over-Voltage 5V	13
4.3 Characterization at $V_{ov} = 6V$	14
4.3.1 Staircase @ $OV=6V$	14
4.3.2 DCR @ $OV=6V$ at different Gate Time from 25 ns to 110 ns	14
4.3.3 DCR @ $OV=6V$ vs Time.....	15
4.3.4 System linearity to evaluate the best operating conditions	16
4.3.5 PDE measurements at Over-Voltage 6V	17
4.4 PDE comparison.....	18
Appendix A: PDE measurement apparatus	19
Appendix B: Block Diagram of the CAEN PSAU	20



1.0 Electrical Characteristics from Data sheet

The layout of this device is shown in Fig. 4. Its main features are reported in Table 3.

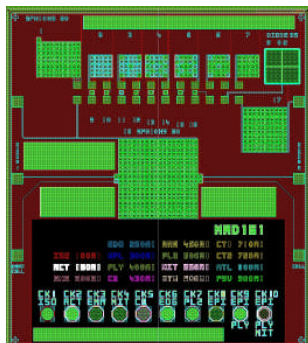



Fig. 1 SPM10H5-60: chip layout.

Table 3 Features of the SPM10H5-60 device.

Parameter	Unit	Value
Sensitive area size	μm^2	1080 × 1080
Cells matrix dimension		18 × 18
Number of cells		324
Cell fill factor	%	67.4
Cell size	μm^2	60 × 60
Quenching resistor squares number		28
Quenching capacitor area	μm^2	26
Cell active area	μm^2	2427
Cell perimetral area	μm^2	844
Bonding pad area	μm^2	150 × 150
Metal grid area (2 pads included)	μm^2	161802

NRD16 – Multichip – SPM10H5_60 BONDING

Electrode	Pin
Cathode	1
Cathode Diode	2
Anode (Back)	10

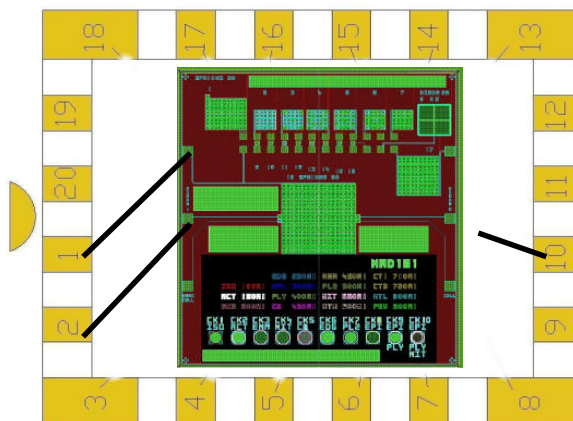



2.0 Breakdown Voltage

The V_{BD} was measured from the voltage-current measurements and tracing the intercept between the line of best fit (range from 1mA to 2mA) and the x-axis.

Here follows the plot of the I-V characteristic

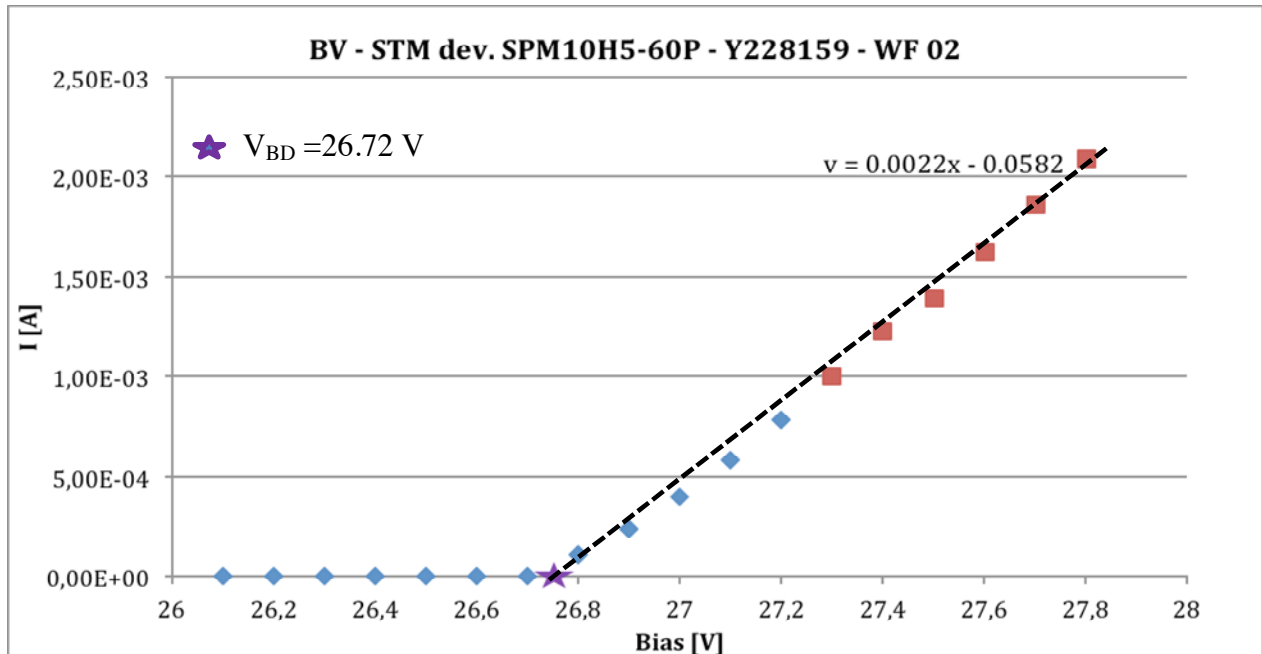


Fig. 1 – BreakDown Voltage @ $T=25.0^{\circ}\text{C}$.


Then the break-down voltage for this SiPM is 26.72 V.



3.0 Staircase and Cross-talk versus Over-Voltage SiPM SPM10H5-60P

The Crosstalk is evaluated by the ratio of the DCR at 1.5 pe- and at 0.5 pe-.


V_{ov}=4.0V

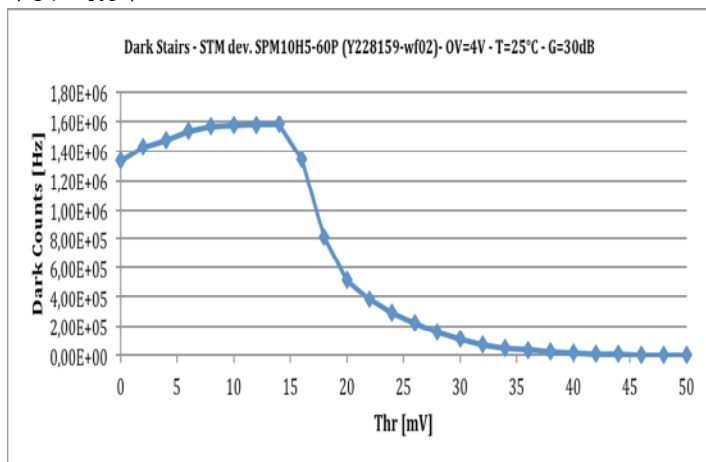

From the data we derive:

Xtalk=1.06% Dark= 1.6 MHz @0.5 pe


V_{ov}=5.0V

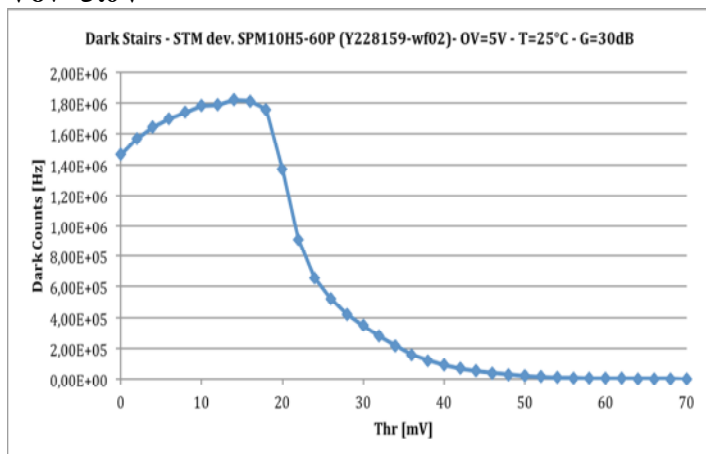

From the data we derive:

Xtalk=0.65% Dark= 1.8 MHz @0.5 pe

V_{ov}=6.0V

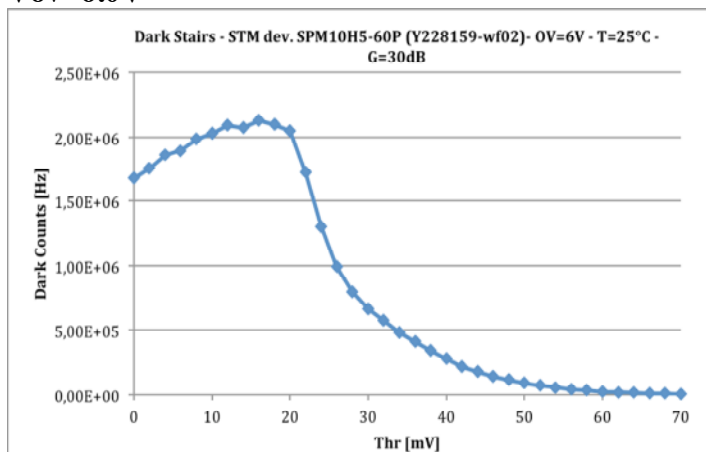

From the data we derive:

Xtalk=0.84% Dark= 2.1 MHz @0.5 pe



4.0 Electro-optical characterization

We characterize the SiPM at three different Over-voltages 4V, 5V and 6V.

The characterization includes the following steps:

1. the Staircase to select the appropriate threshold,
2. the Dark Count Rate (DCR) at different gate time in order to select the best hold-off time
3. the system linearity to evaluate the best illumination conditions (avoid the saturation)
4. PDE measurements taking into account the results of the previous steps.

4.1 Characterization at $V_{ov} = 4V$

Here will follow the characterization at $V_{ov}=4V$.

4.1.1 Staircase @ $OV=4V$

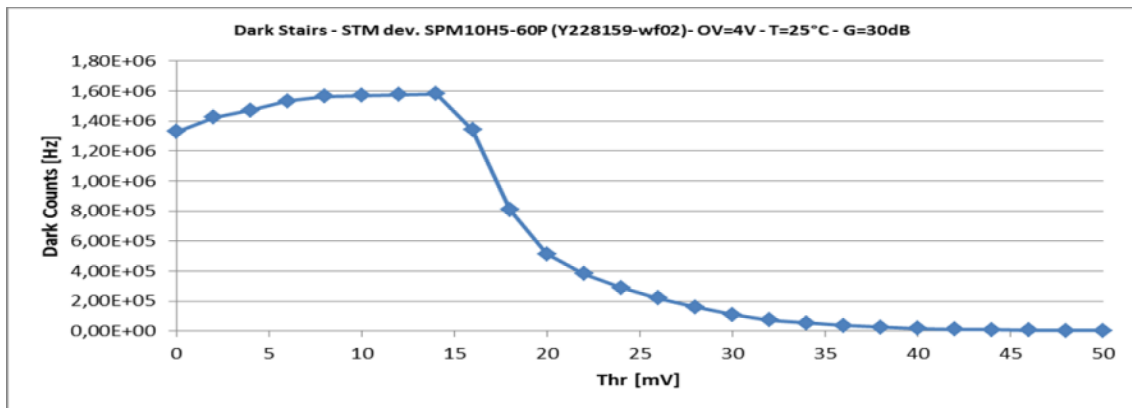


Fig. 2 – Dark Stair versus V_{thr} @ $T=25.0^{\circ}C$.

From this plot we derived a V_{thr} of -10 mV .

4.1.2 DCR @ $OV=4V$ at different Gate Time from 25 ns to 110 ns

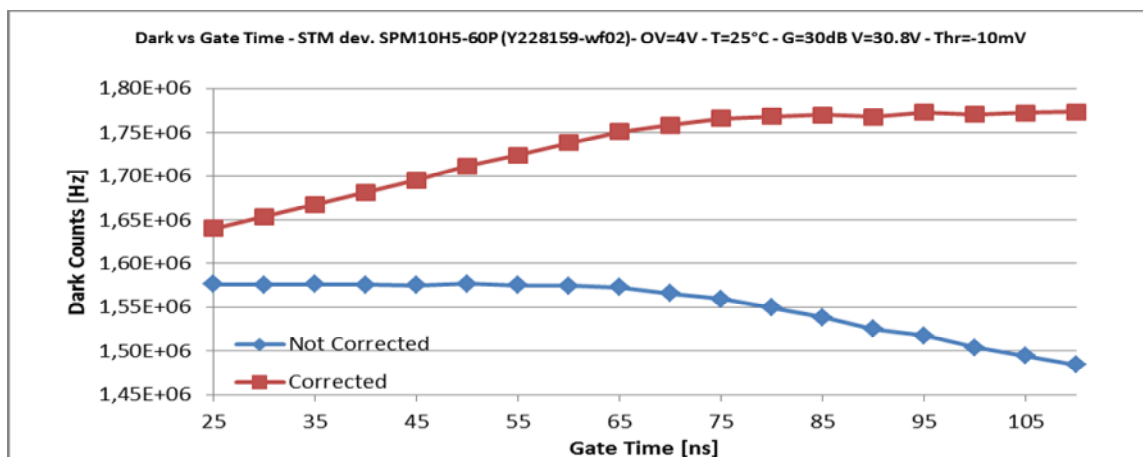


Fig.3 - DARK vs GATE TIME $V_{ov}=4V$ - $Thr=-10\text{ mV}$ $T=25^{\circ}$. Measurements were performed at gate times from 25ns to 110ns. The upper curve is obtained correcting for dead time the lower curve. Temperature compensation for gain stabilization is also adopted

We select as optimal Gate Time - : $\rightarrow \tau = 90\text{ ns}$



4.1.2 DCR @ OV=4V vs Time

By selecting the above the threshold level and the gate time obtained in the previous subsections, a measure of dark versus time is carried out.


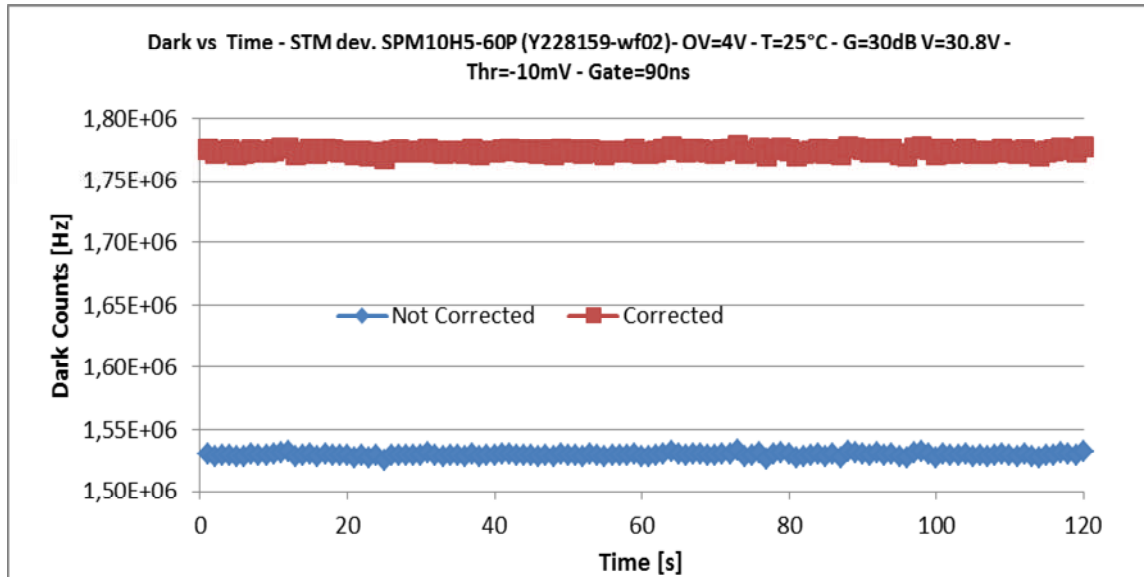


Fig.4 - DARK vs Time $V_{ov}=4V$ - $Thr=-10\text{ mV}$ $T=25^\circ$ The upper curve is obtained correcting for dead time the lower curve. Temperature compensation for gain stabilization is also adopted.

From this plot we derive that at a $V_{ov}=4V$ and with a threshold of 0.5 pe the effective **DCR @ 25°C is 1.77 MHz.**



4.1.4 System linearity to evaluate the best operating conditions

To characterize the SiPM by using the best illumination conditions, that means avoiding the system saturation and maintaining a sufficient signal on the NIST calibrated photodiode, linearity measurements were carried out. Furthermore the non-linearity conditions were tested by using the PDE measurements at a selected wavelength.

Here will follow the obtained plots of the signal count rate versus the photodiode current @520 nm and the PDE @520 nm versus the signal count rate.

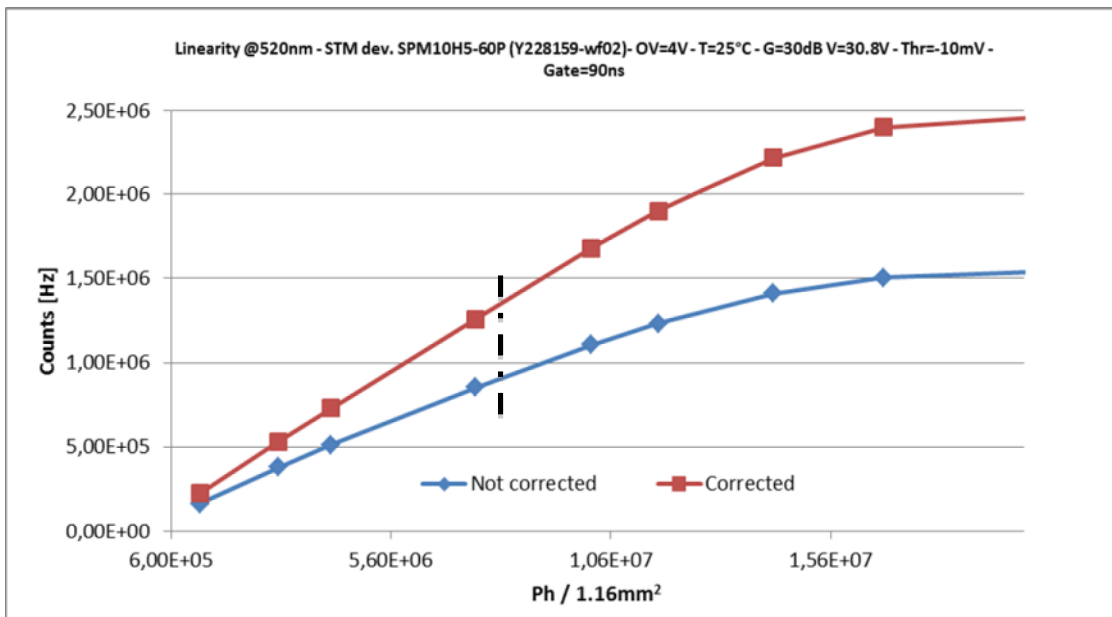


Fig. 5 – Linearity at 520 nm with and without the dead time correction.

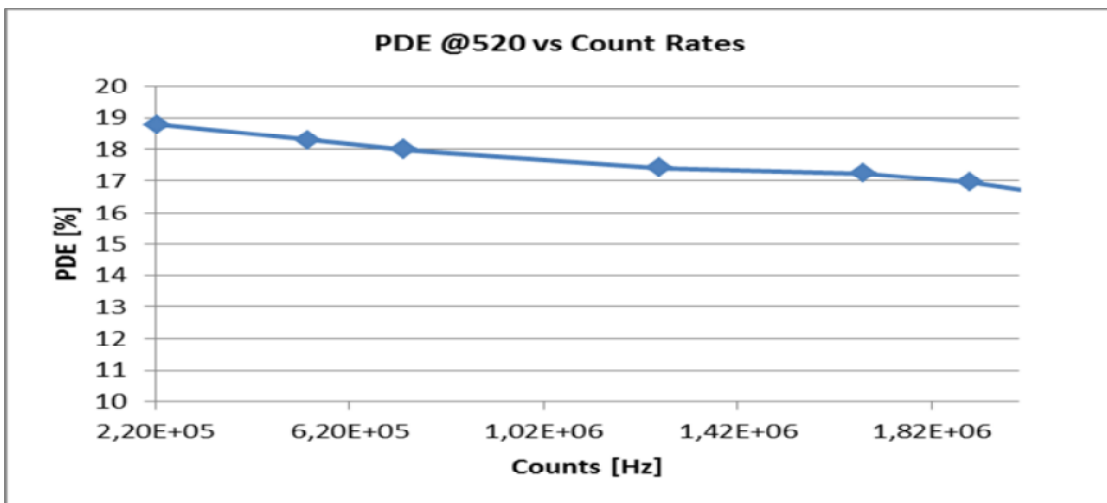


Fig.6 – PDE measurements at 520nm versus counts, from 220 KHz to 1800KHz operating the SiPM at $V_{ov}=4V$ $T=25^{\circ}C$, $V_{thr}=-10$ mV, Gate time=90 ns

From these plots we derive that the system shows a not-linearity behavior at rates greater than 850 KHz uncorrected corresponding at about 1.3 MHz corrected for dead time. And the PDE is about 18-19 % in the range of 220 KHz – 1.0 MHz without dark counts (Fig.6)

Then, to be conservative, the PDE measurements have to be carried out with **uncorrected signals and without DCR subtraction not higher than 2.3 MHz corresponding to 2.8 MHz corrected for dead time.**



4.1.5 PDE measurements at Over-Voltage 4V

Measurements were performed at $V_{OV} = 4V$ and gate time 90ns. The plot reports the PDE with values corrected for the Dead Time.

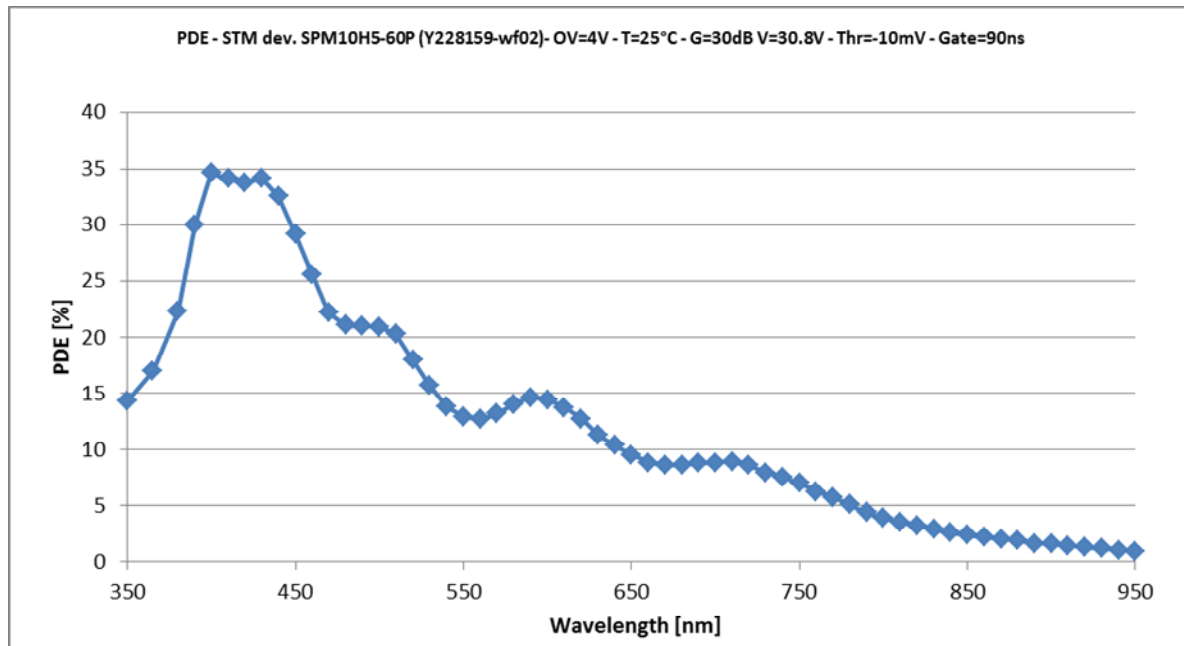


Fig.7 – PDE measurements operating the SiPM at $V_{ov}=4V$ $T=25^{\circ}C$, $V_{thr}=-10$ mV, Gate time=90 ns



4.2 Characterization at $V_{ov} = 5V$

Here will follow the characterization at $V_{ov}=5V$.

4.2.1 Staircase @ $OV=5V$

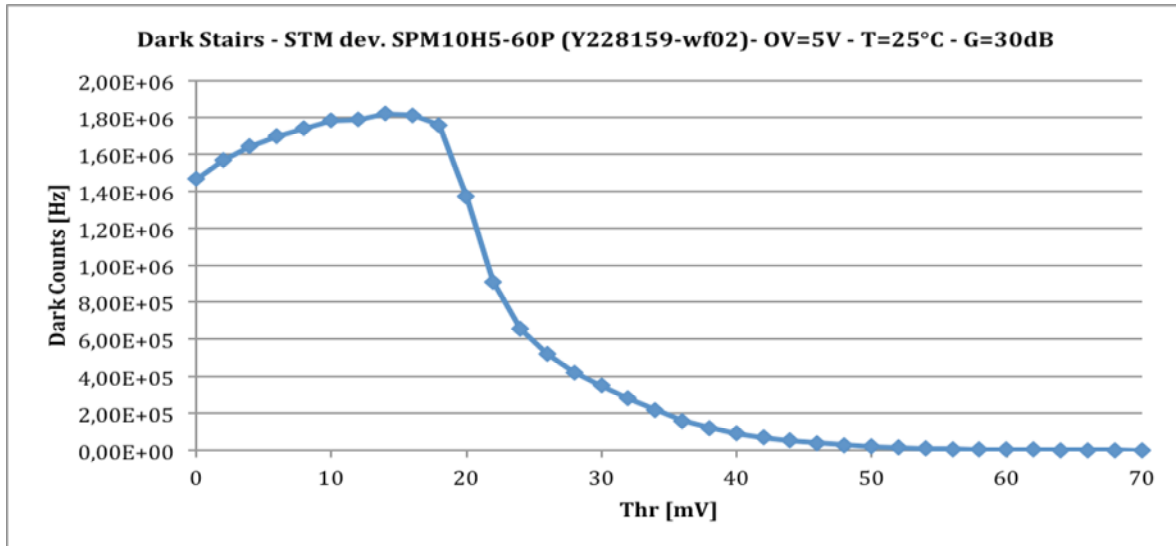


Fig. 8 – Dark Stair versus V_{thr} @ $T=25.0^{\circ}C$.

From this plot we derived a V_{thr} of -12 mV .

4.2.2 DCR @ $OV=5V$ at different Gate Time from 25 ns to 110 ns

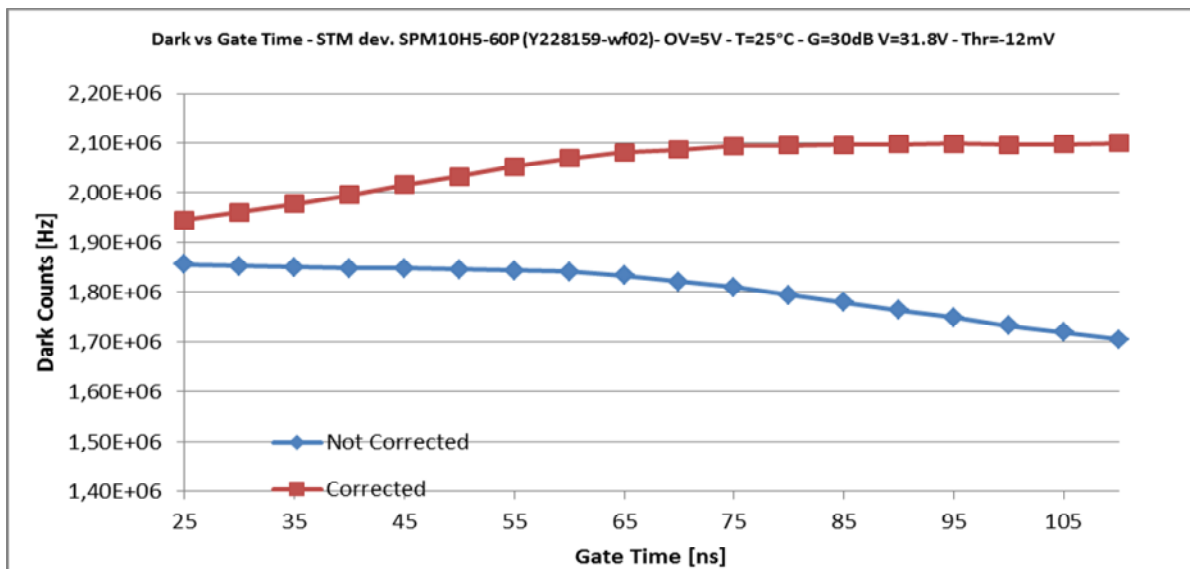


Fig.9 - DARK vs GATE TIME $V_{ov}=5V$ - $Thr=-12\text{ mV}$ $T=25^{\circ}$. Measurements were performed at gate times from 25ns to 110ns. The upper curve is obtained correcting for dead time the lower curve. Temperature compensation for gain stabilization is also adopted.

We select as optimal Gate Time - : $\rightarrow \tau = 90\text{ ns}$



4.2.3 DCR @ OV=5V vs Time

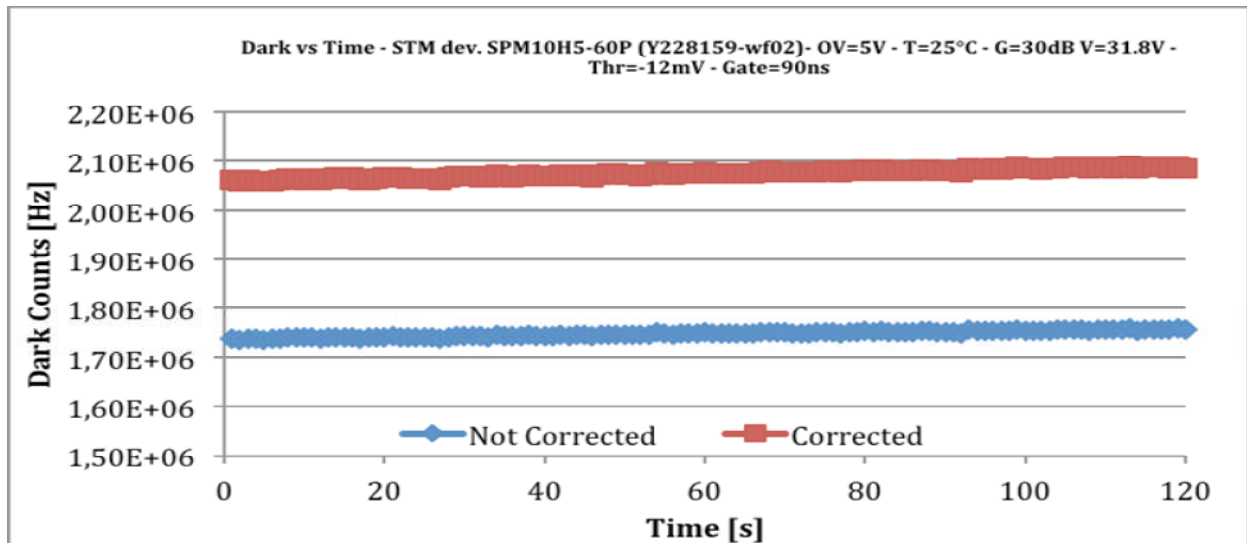


Fig.10 - DARK vs Time $V_{ov}=5V$ - $Thr=-12\text{ mV}$ $T=25^\circ$. The upper curve is obtained correcting for dead time the lower curve. Temperature compensation for gain stabilization is also adopted.

From this plot we derive that at a $V_{ov}=5V$ and with a threshold of 0.5 pe the effective **DCR @ 25°C is 1.9 MHz**.



4.2.4 System linearity to evaluate the best operating conditions

To characterize the SiPM by using the best illumination conditions, that means avoiding the system saturation and maintaining a sufficient signal on the NIST calibrated photodiode, linearity measurements were carried out. Furthermore the non-linearity conditions were tested by using the PDE measurements at a selected wavelength.

Here will follow the obtained plots of the signal count rate versus the photodiode current @520 nm and the PDE @520 nm versus the signal count rate.

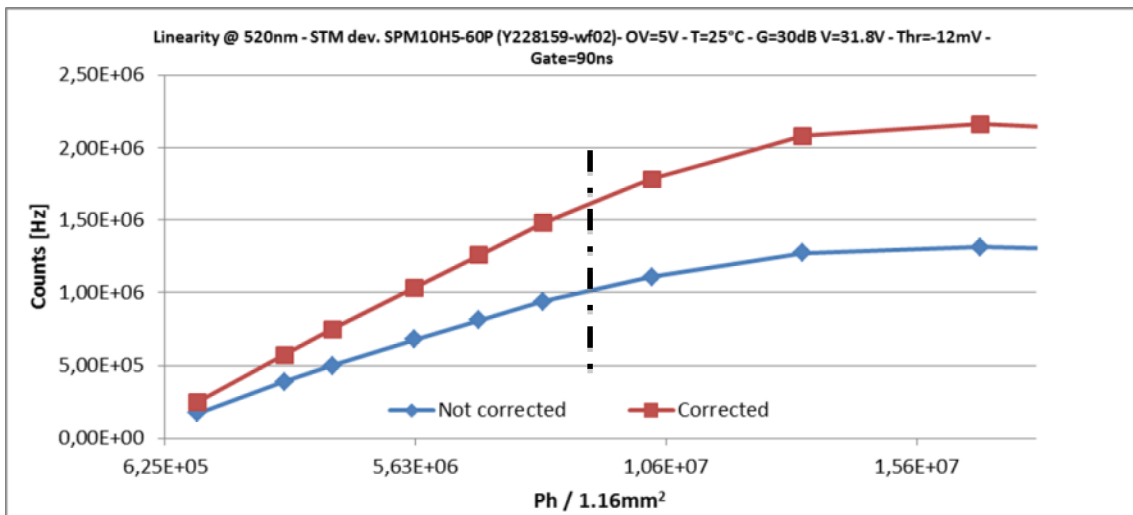


Fig. 11 – Linearity at 520 nm with and without the dead time correction.

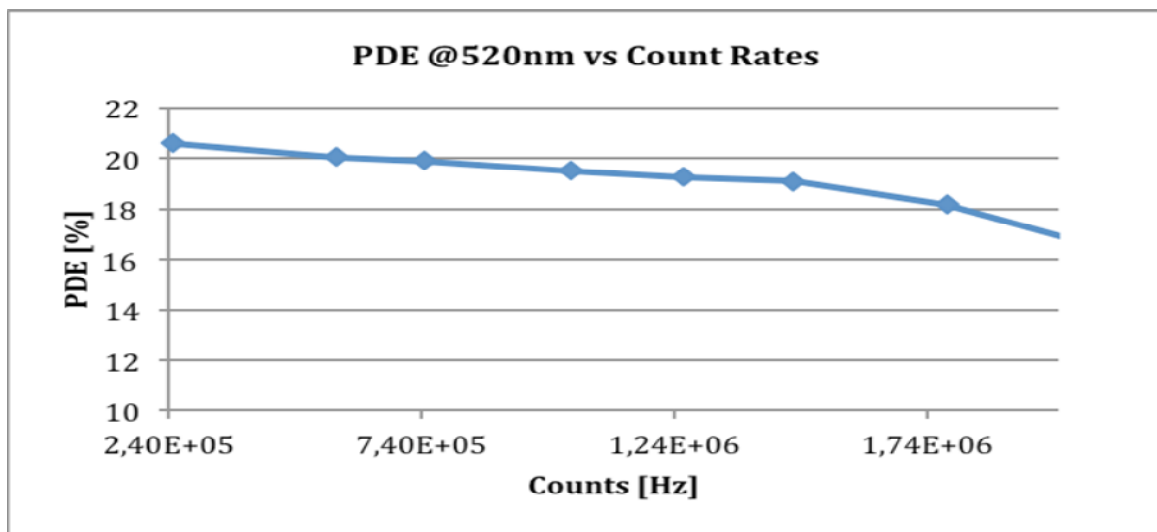


Fig.12 – PDE measurements at 520 nm versus counts from 240KHz to 1700KHz operating the SiPM at $V_{ov}=5V$ $T=25^{\circ}C$, $V_{thr}=-12$ mV, Gate time=90 ns

From these plots we derive that the system shows a not-linearity behavior at counts greater than 800 KHz uncorrected corresponding at about 1.3MHz corrected for dead time. And the PDE is about 19.2-21 % in the range of 240 – 1.25 KHz without dark counts (Fig.12).

Then, to be conservative, the PDE measurements have to be carried out with **uncorrected signals and without DCR subtraction not higher than 2.6 MHz corresponding to 3.0 MHz corrected for dead time.**



4.2.5 PDE measurements at Over-Voltage 5V

Measurements were performed at $V_{OV} = 5V$ and gate time 90ns.
The plot reports the PDE with values corrected for the Dead Time.

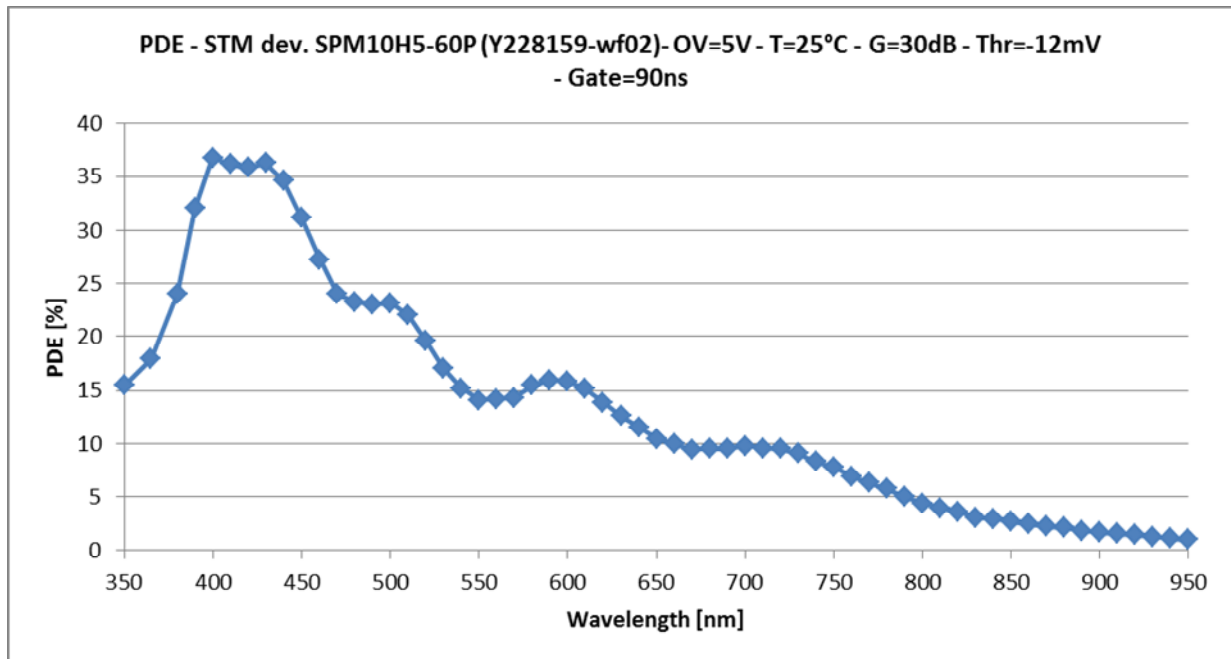


Fig.13 – PDE measurements operating the SiPM at $V_{ov}=5V$ $T=25^{\circ}C$, $V_{thr}=-12$ mV, Gate time=90 ns



4.3 Characterization at $V_{ov} = 6V$

Here will follow the characterization at $V_{ov}=6V$.

4.3.1 Staircase @ $OV=6V$

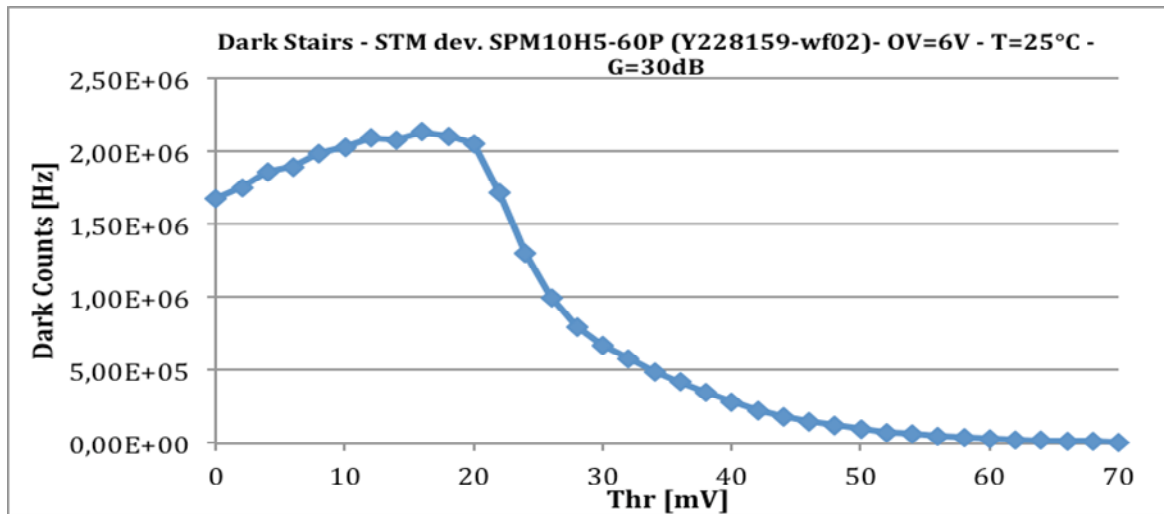


Fig. 14 – Dark Stair versus V_{thr} @ $T=25.0^{\circ}C$.

From this plot we derived a V_{thr} of $-14 mV$.

4.3.2 DCR @ $OV=6V$ at different Gate Time from 25 ns to 110 ns

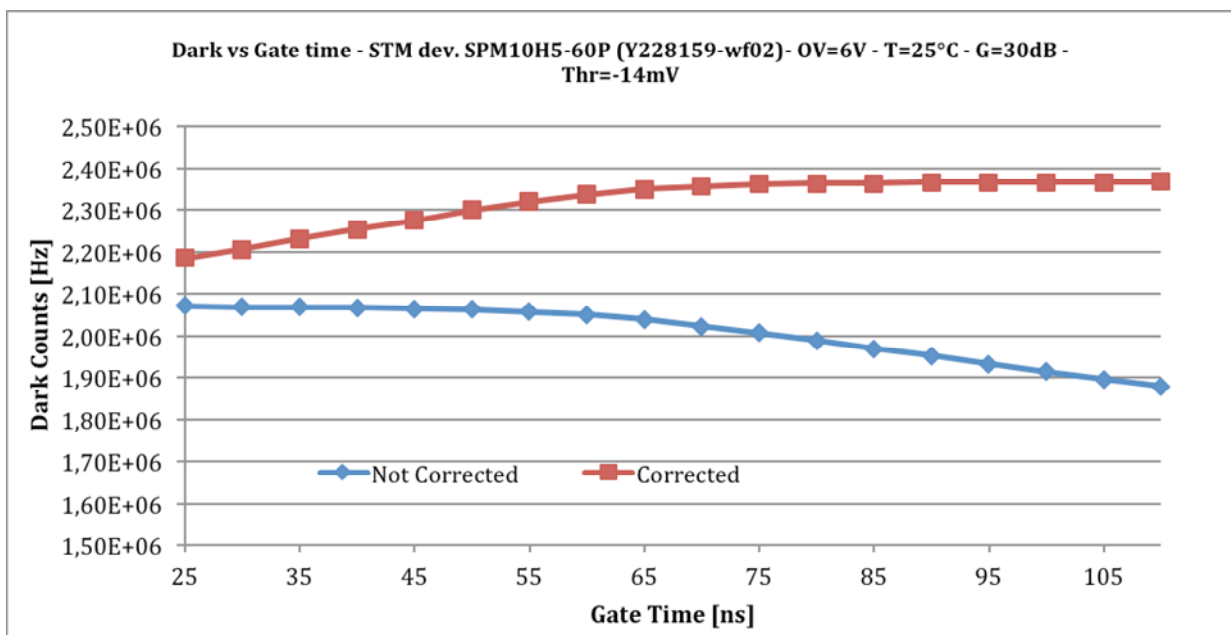


Fig.15 - DARK vs GATE TIME $V_{ov}=6V$ - $Thr=-14 mV$ $T=25^{\circ}$ Measurements were performed at gate times from 25ns to 110ns. The upper curve is obtained correcting for dead time the lower curve. Temperature compensation for gain stabilization is also adopted.

We select as optimal Gate Time - : $\rightarrow \tau = 90 ns$



4.3.3 DCR @ OV=6V vs Time

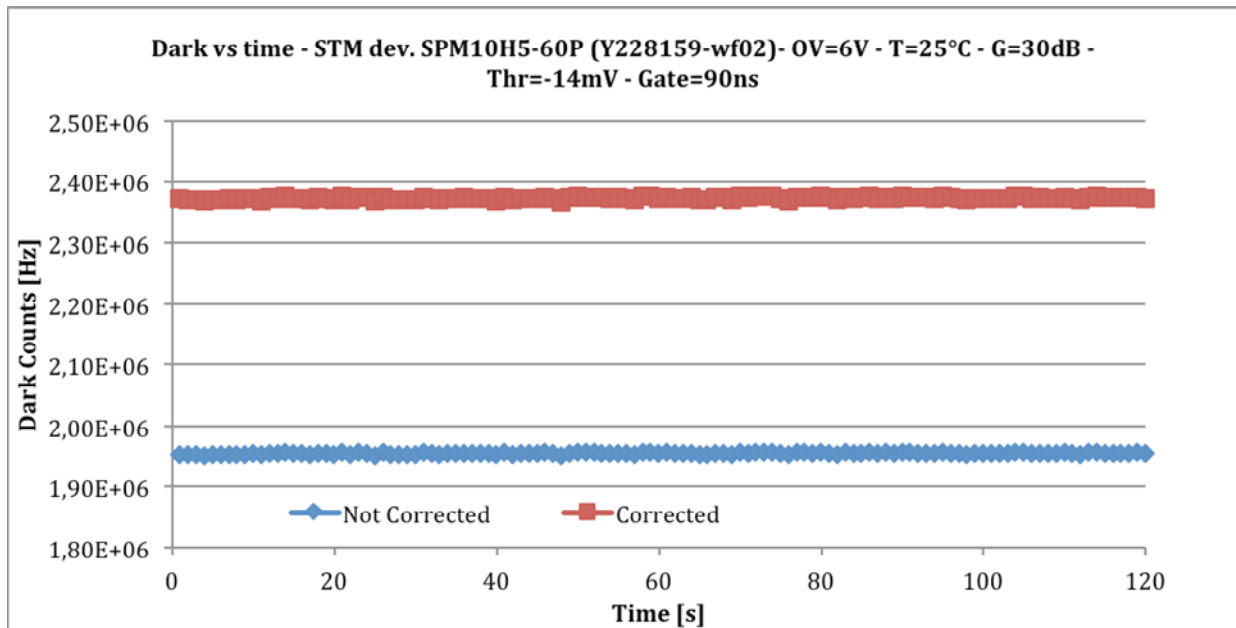


Fig.16 - DARK vs Time $V_{ov}=6V$ - $Thr=-14\text{ mV}$ $T=25^\circ$ The upper curve is obtained correcting for dead time the lower curve. Temperature compensation for gain stabilization is also adopted.

From this plot we derive that at a $V_{ov}=6V$ and with a threshold of 0.5 pe the effective **DCR @ 25°C is 2.35 MHz**.



4.3.4 System linearity to evaluate the best operating conditions

To characterize the SiPM by using the best illumination conditions, that means avoiding the system saturation and maintaining a sufficient signal on the NIST calibrated photodiode, linearity measurements were carried out. Furthermore the non-linearity conditions were tested by using the PDE measurements at a selected wavelength. Here will follow the obtained plots of the signal count rate versus the photodiode current @520 nm and the PDE @520 nm versus the signal count rate.

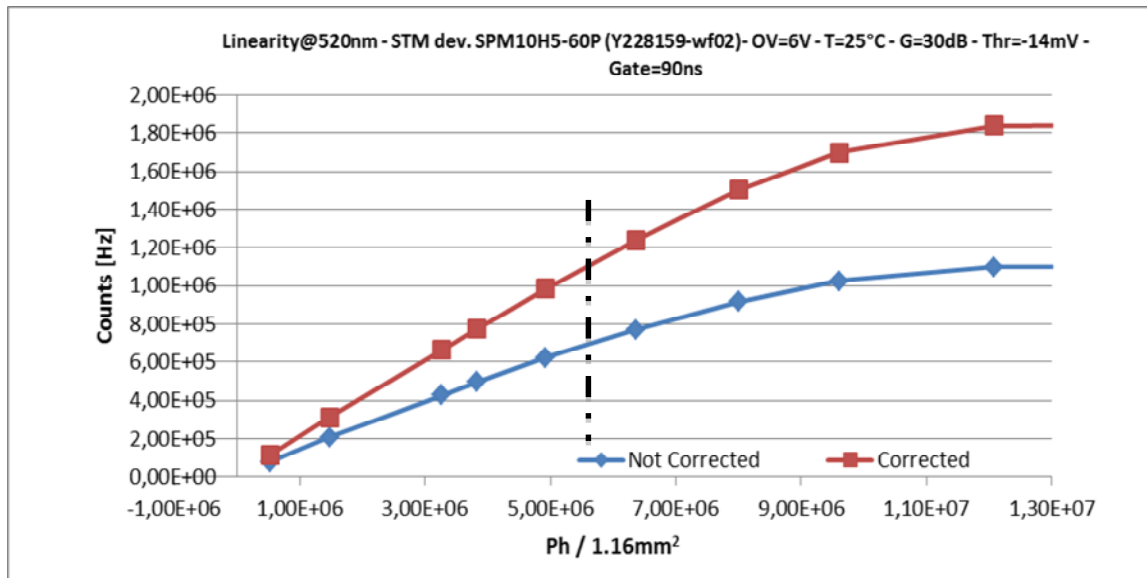


Fig. 17 – Linearity at 520 nm with and without the dead time correction.

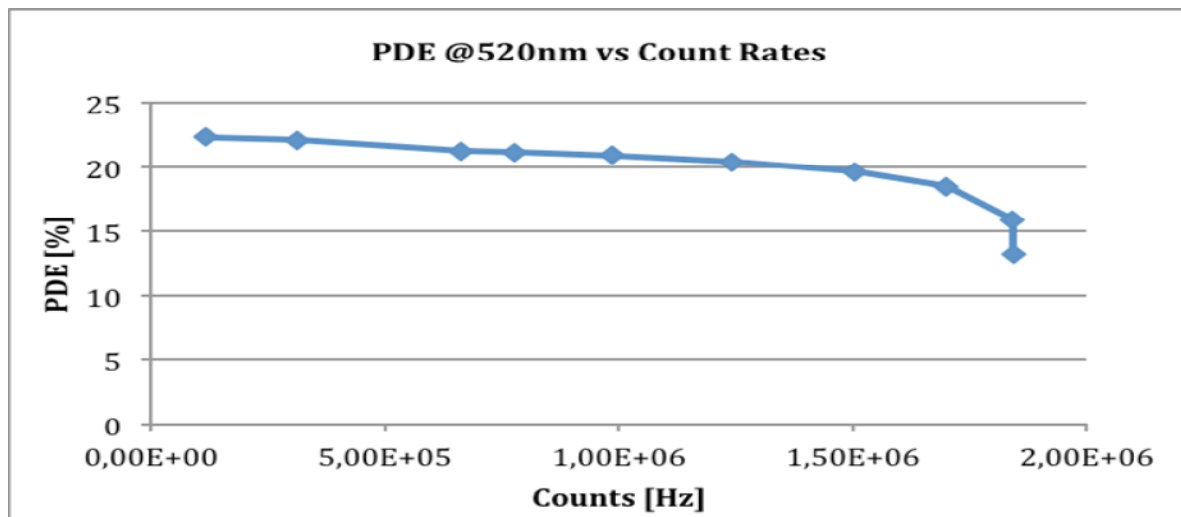


Fig.18 – PDE measurements at 520nm versus counts from 250KHz to 1500KHz operating the SiPM at $V_{ov}=6V$ $T=25^\circ C$, $V_{thr}=-14$ mV, Gate time=90 ns

From these plots we derive that the system shows a not-linearity behavior at counts greater than 600 KHz uncorrected corresponding at about 1.0 MHz corrected for dead time. And the PDE is about 21-23 % in the range of 250 – 1.0 MHz without dark counts (Fig.19)

Then, to be conservative, the PDE measurements have to be carried out with **uncorrected signals and without DCR subtraction not higher than 2.6 MHz corresponding to 3.0 MHz corrected for dead time.**



4.3.5 PDE measurements at Over-Voltage 6V

Measurements were performed at $V_{OV} = 6V$ and gate time 90ns. The plot reports the PDE with values corrected for the Dead Time.

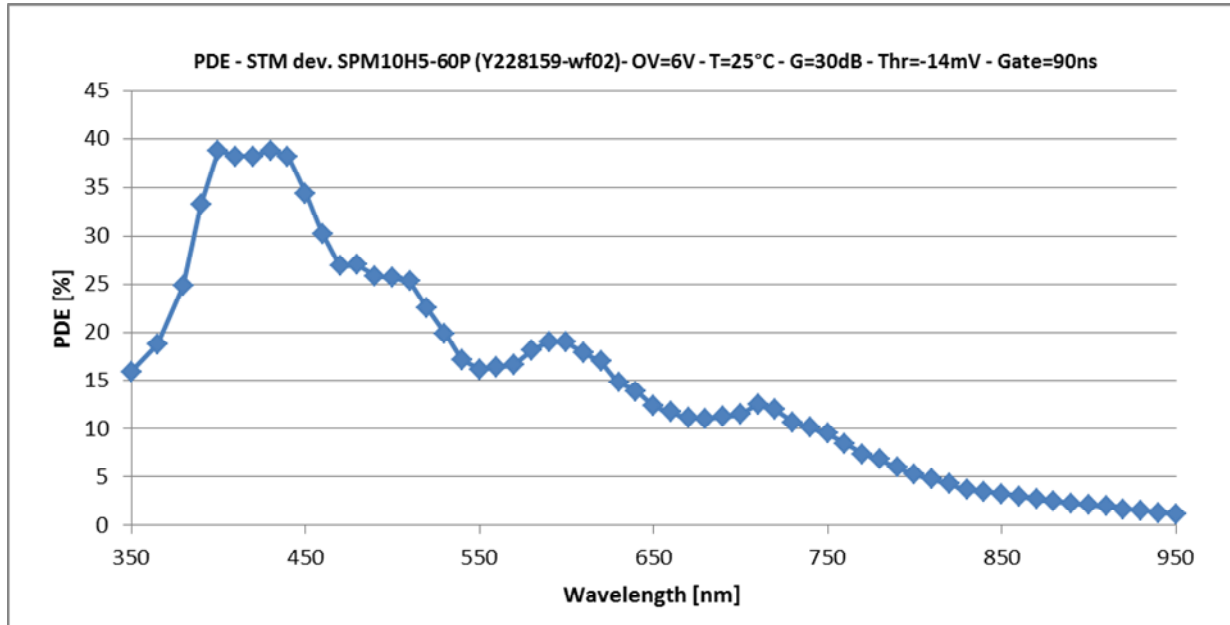


Fig.20 – PDE measurements operating the SiPM at $V_{ov}=6V$, $T=25^{\circ}C$, $V_{thr}=-14$ mV, Gate time=90 ns



4.4 PDE comparison

PDE measurements at the various Over Voltages are here compared.

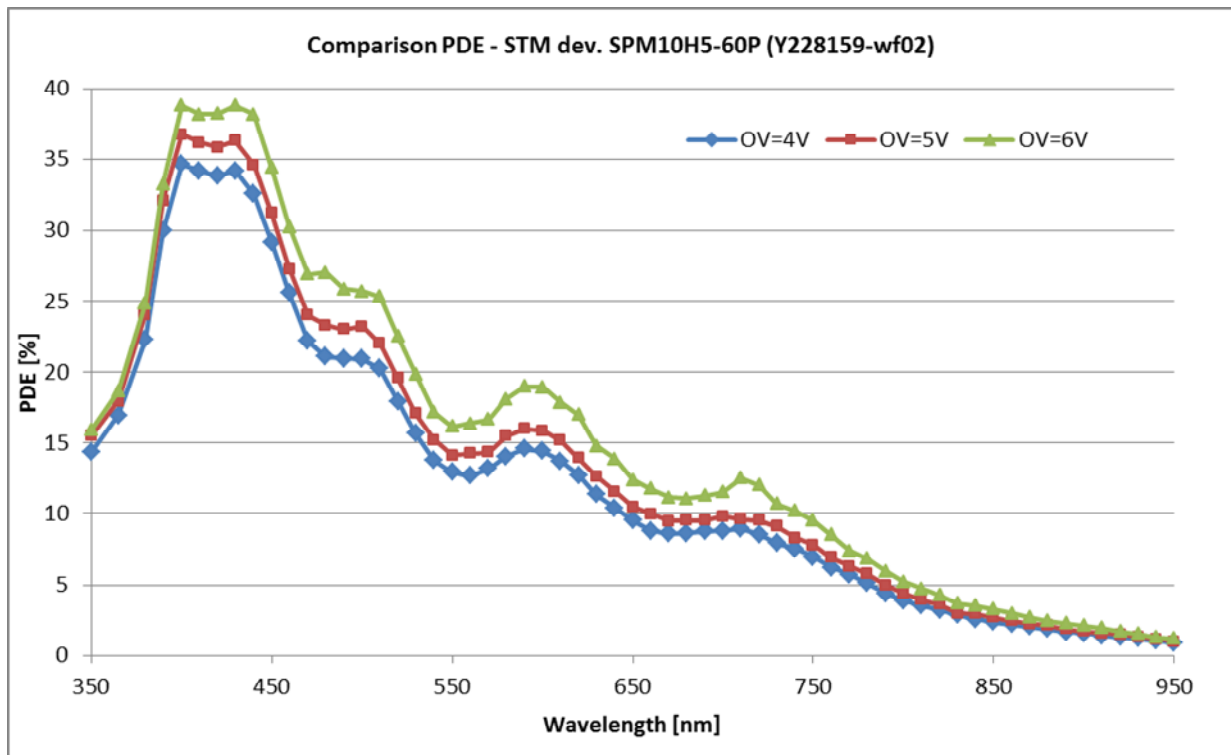


Fig.21– PDE measurements comparison at $V_{ov}=4.0V$, $V_{ov}=5.0V$ and $V_{ov}=6.0V$ @ $T=25^{\circ}C$.

Appendix A: PDE measurement apparatus

PDE measurements Apparatus

